

Stationary Phase: **EtG/EtS**


Raptor

LC Columns

Selectivity Accelerated

All Matrix Interferences Resolved

How often are matrix interferences affecting your EtG/EtS analysis? Restek's EtG/EtS solution consistently resolves analytes away from matrix interferences in a fast, 4-minute, dilute-and-shoot method.

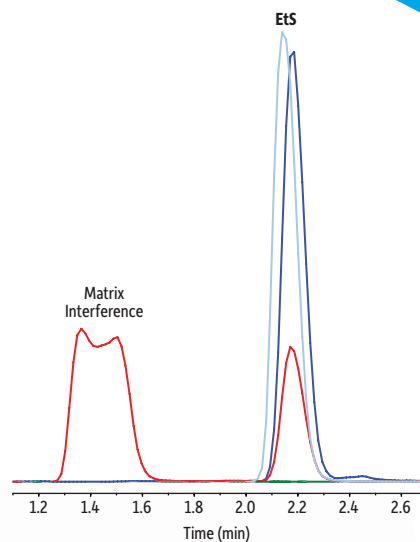

RESTEK

Pure Chromatography

www.restek.com/raptor

Raptor EtG/EtS Column

- Proven performance for accurate, reliable ethyl glucuronide (EtG) and ethyl sulfate (EtS) analysis.
- Strong retention consistently resolves analytes from matrix interferences.
- Long column lifetime ensures consistent performance injection after injection.
- Fast, 4-minute, dilute-and-shoot LC-MS/MS analysis supports high sample throughput.

Switch to a Raptor EtG/EtS column when you need consistent resolution of EtG and EtS from matrix interferences and long column lifetimes.

Order yours today at www.restek.com/raptor

Part of Restek's Raptor LC column line featuring SPP core-shell silica:

- Higher efficiency and resolution for drastically faster analysis times.
- Increased sample throughput with existing HPLC instrumentation
- Long-lasting ruggedness for dependable reproducibility.

Column Description

Pore Size:

90 Å

Particle:

2.7 µm superficially porous silica (SPP or "core-shell")

Surface Area:

130 m²/g

End-Cap:

Proprietary

Carbon Load:

Proprietary

USP Phase Code:

NA

Phase Category:

Proprietary

Ligand Type:

Proprietary

Recommended Usage:

pH Range: 2.0–8.0

Maximum Temperature: 40 °C

Maximum Pressure: 600 bar/8,700 psi



Properties:

- Resolution of EtG and EtS from matrix interferences.
- Increased retention of EtG and EtS compared to traditional phases.

Switch to a Raptor EtG/EtS when:


- Other columns can't resolve EtG and EtS from matrix components.
- You need high-throughput EtG/EtS analysis.
- Low-level detection limits are desired.



Definitive Results for Alcohol Monitoring

Restek has developed a new Raptor column that significantly improves EtG and EtS analysis for alcohol monitoring programs. The Raptor EtG/EtS column consistently retains and resolves these important biomarkers from matrix interferences, providing accurate, reliable results injection after injection (Figure 1). Dependable performance, a fast 4-minute analysis, and long column lifetime make this column ideal for high-throughput labs. Paired with our quality reference standards and the optimized, validated method shown below, Restek's Raptor EtG/EtS column is part of a complete solution that will help testing labs save time and increase certainty.

Figure 1: Rugged Raptor EtG/EtS columns provide complete resolution and consistent results even after 1,000 injections, allowing more samples to be analyzed between column changes.

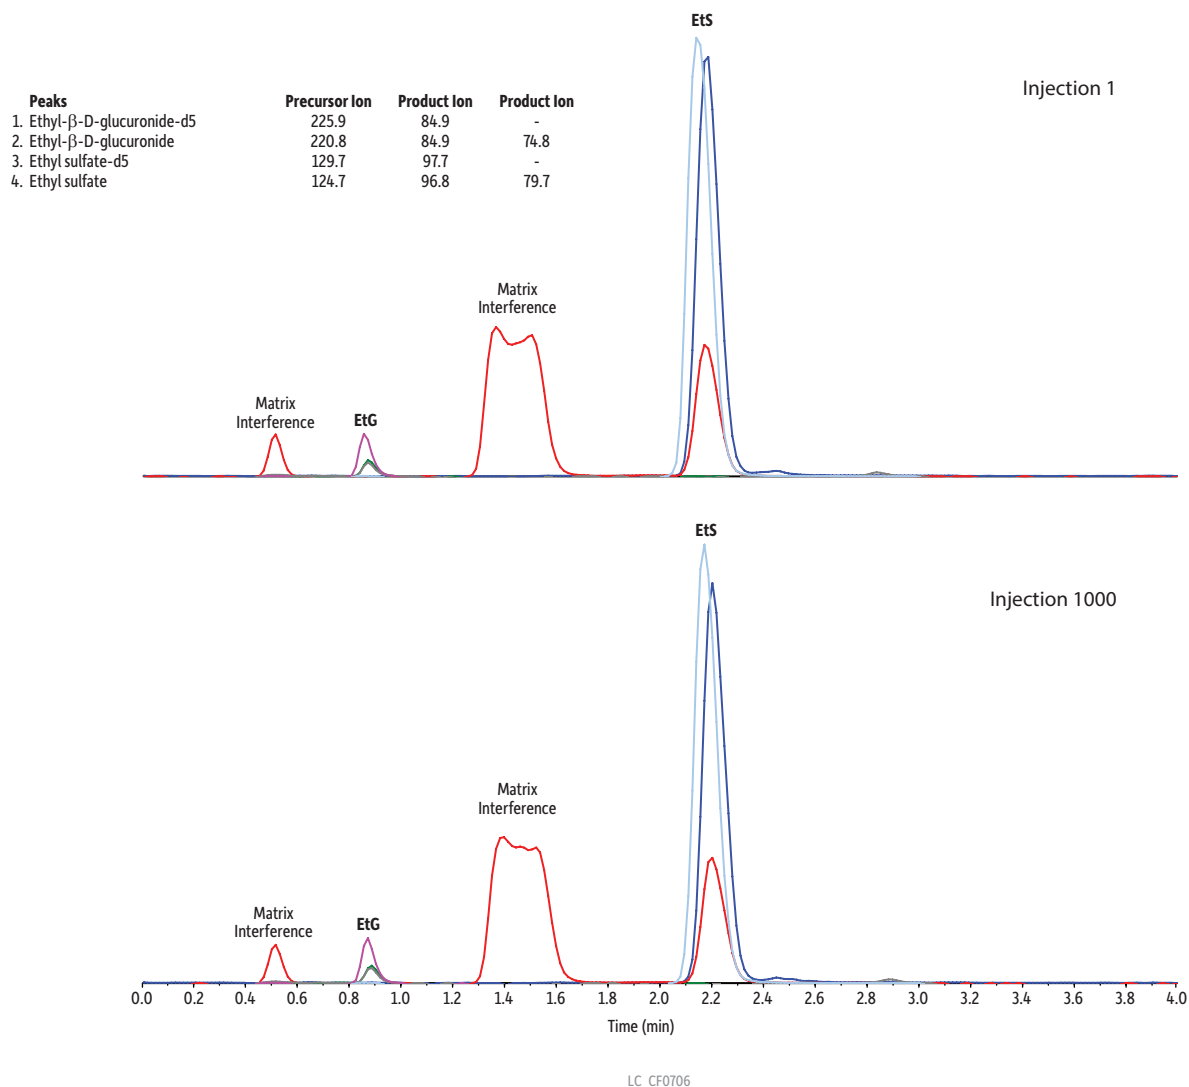

Column: Raptor EtG/EtS (cat.# 9325A12); Dimensions: 100 mm x 2.1 mm ID, Particle Size: 2.7 μm; Guard Column: UltraShield UHPLC precolumn filter, 0.2 μm frit (cat.# 25809); Temp.: 35 °C; Sample: A 500 ng/mL QC sample was prepared in urine. 50 μL of the sample was diluted with 950 μL of a working internal standard (25 ng/mL EtS-d5/100 ng/mL EtG-d5 in 0.1% formic acid in water). The sample was vortexed at 3,500 rpm for 10 seconds to mix. The sample was then centrifuged at 3,000 rpm for 5 minutes at 10 °C. The autosampler needle was adjusted to inject from the supernatant. Inj. Vol.: 10 μL; Mobile Phase: A: 0.1% Formic acid in water; B: 0.1% Formic acid in acetonitrile; Gradient (%B): 0.00 min (5% B), 2.50 min (35% B), 2.51 min (5% B), 4.00 (5% B); Flow: 0.5 mL/min; Detector: MS/MS; Ion Mode: ESI-; Mode: MRM; Instrument: HPLC; Notes: The following reference standards were used: ethyl-β-D-glucuronide (cat.# 34101), ethyl-β-D-glucuronide-d5 (cat.# 34102), ethyl sulfate sodium salt (cat.# 34103), ethyl sulfate-d5 sodium salt (cat.# 34104).

Struggling with EtG/EtS matrix interferences? Here's your solution!



Raptor EtG/EtS LC Column

- Proven performance for accurate, reliable ethyl glucuronide (EtG) and ethyl sulfate (EtS) analysis.
- Strong retention consistently resolves analytes from matrix interferences.
- Long column lifetime ensures consistent performance injection after injection.
- Fast, 4-minute, dilute-and-shoot LC-MS/MS analysis supports high sample throughput.
- Save time and increase certainty with Restek's definitive EtG/EtS method and quality reference standards.

ID	Length	qty.	cat.#
2.7 µm			
2.1 mm	100 mm	ea.	9325A12

UltraShield UHPLC PreColumn Filter

- Cost-effective protection for UHPLC systems.
- Reliable way to filter out particulates and extend column lifetime.
- Minimize extra column volume and maximize UHPLC sample throughput vs. guard cartridges.
- Connects easily to any column with Parker-style ports; not compatible with Waters columns.
- Leak tight to 15,000 psi (1,034 bar).
- 0.5 µm or 0.2 µm stainless-steel frit in a stainless-steel body with PEEK ferrule.



Description	Porosity	qty.	cat.#
	0.2 µm frit	ea.	25809
UltraShield UHPLC PreColumn Filter	0.2 µm frit	5-pk.	25810
	0.2 µm frit	10-pk.	25811

EtG and EtS Standards

- Alcohol metabolite biomarkers for monitoring alcohol consumption in urine samples.
- Available as unlabeled standards for instrument calibration and as deuterated internal standards for sample analysis.
- Verified composition and stability.
- Pair with Restek's definitive EtG/EtS method and Raptor EtG/EtS LC column for accurate, reliable results.



Description	CAS #	Conc. in Solvent	Certified Reference Material?	Max Shelf Life on Ship Date	Min Shelf Life on Ship Date	cat.#
Ethyl-β-D-glucuronide (EtG)	17685-04-0	1,000 µg/mL in methanol, 1 mL/ampul	Yes	36 months	6 months	34101 (ea.)
Ethyl-β-D-glucuronide-d5 (EtG-d5)	1135070-98-2	1,000 µg/mL in methanol, 1 mL/ampul	Yes	36 months	6 months	34102 (ea.)
Ethyl sulfate sodium salt (EtS)	546-74-7	1,000 µg/mL in methanol, 1 mL/ampul	Yes	36 months	6 months	34103 (ea.)
Ethyl sulfate-d5 sodium salt (EtS-d5)	1329611-05-3	1,000 µg/mL in methanol, 1 mL/ampul	Yes	36 months	6 months	34104 (ea.)

Experience *Selectivity Accelerated*. Order the Raptor EtG/EtS today at www.restek.com/raptor

RESTEK
Pure Chromatography

Questions? Contact us or your local Restek representative (www.restek.com/contact-us).

Restek patents and trademarks are the property of Restek Corporation. (See www.restek.com/Patents-Trademarks for full list.) Other trademarks in Restek literature or on its website are the property of their respective owners. Restek registered trademarks are registered in the U.S. and may also be registered in other countries. To unsubscribe from future Restek communications or to update your preferences, visit www.restek.com/subscribe To update your status with an authorized Restek distributor or instrument channel partner, please contact them directly.

© 2020 Restek Corporation. All rights reserved. Printed in the U.S.A.

www.restek.com



Lit. Cat.# CF5S2741B-UNV